


## Tube Labelling

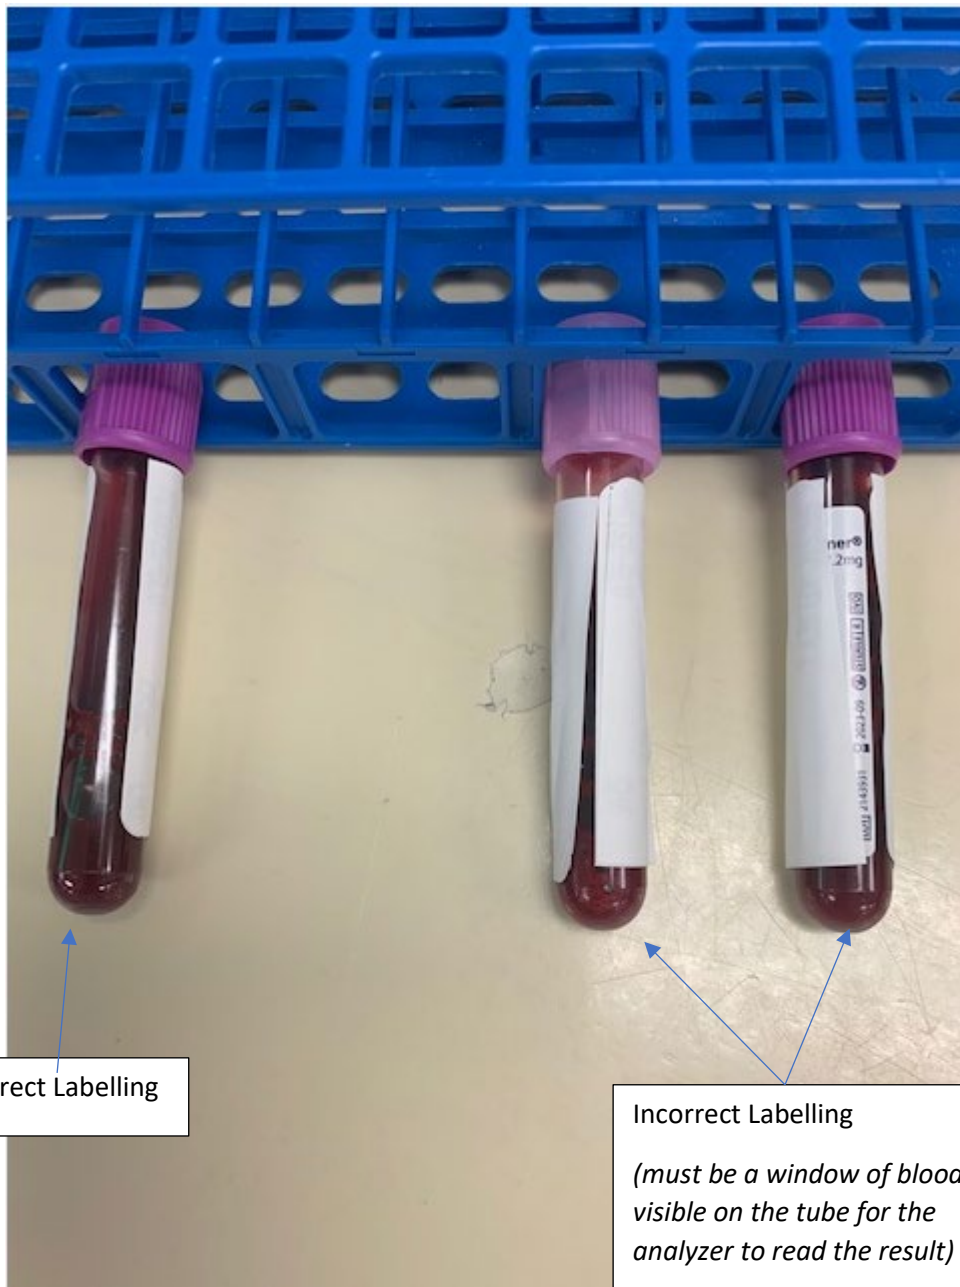

Correct Labelling

Incorrect Labelling

*(must be a window of blood visible on the tube for the analyzer to read the result)*